




CE
1936

dish 35/70/100

Containers for the preparation of platelet gel and fibrin gel

INSTRUCTIONS FOR USE

NOTE: THESE DEVICES MUST BE USED EXCLUSIVELY IN COMBINATION WITH PLATELTEX ACT.

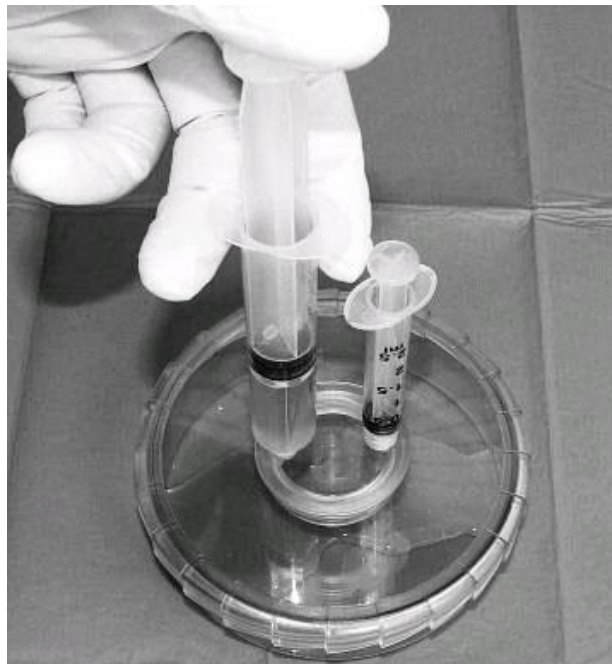

Please follow the instructions of PLATELTEX ACT, using these sterile containers as specified

Recommendations for a correct use of the set

Plateltex Dish is supplied in a sealed and labeled package. The set contains sterile materials. Never use the product after the expiry date. Store the device in a cool and dry place far from the direct sunlight. Never use the device whenever, during the visual inspection, packaging anomalies were found.

Procedure of waste disposal

Wastes should be disposed in compliance with National and local regulations for the Disposal of Health Wastes.

TABLE OF SYMBOLS

CAUTION	DO NOT REUSE	STERILE EO	KEEP AWAY FROM SUNLIGHT	DATE OF MANUFACTURE	DO NOT RESTERILIZE	CONSULT INSTRUCTIONS FOR USE
-10°C 60°C TEMPERATURE LIMITATION	MANUFACTURER	KEEP DRY	LOT BATCH CODE	DO NOT USE IF PACKAGE IS DAMAGED	USE BY	

Manufacturer:

PLATELTEX S.R.O.
Vlasska 24
11800 Praha 1
Czech Republic

<http://www.plateltex.com> info@plateltex.com